

FIG. 2

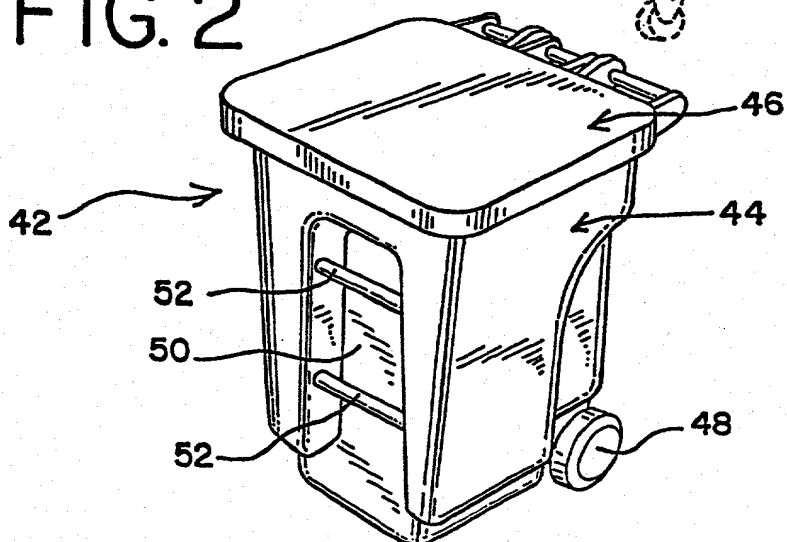


FIG. 3 is a perspective view of the device in a first position, showing the handle 78 and the base 70. FIG. 4 is a perspective view of the device in a second position, showing the handle 78 and the base 70. FIG. 3a is a cross-sectional view of the device in the first position, showing the internal components. FIG. 4a is a cross-sectional view of the device in the second position, showing the internal components.

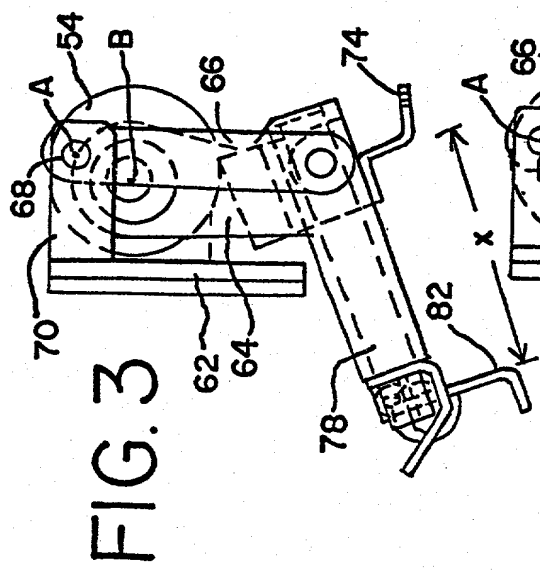


FIG. 3

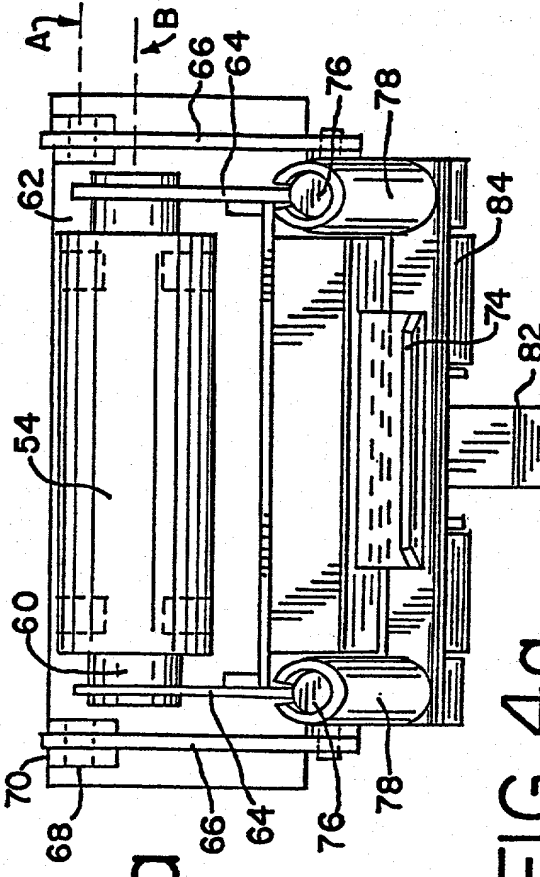


FIG. 3a


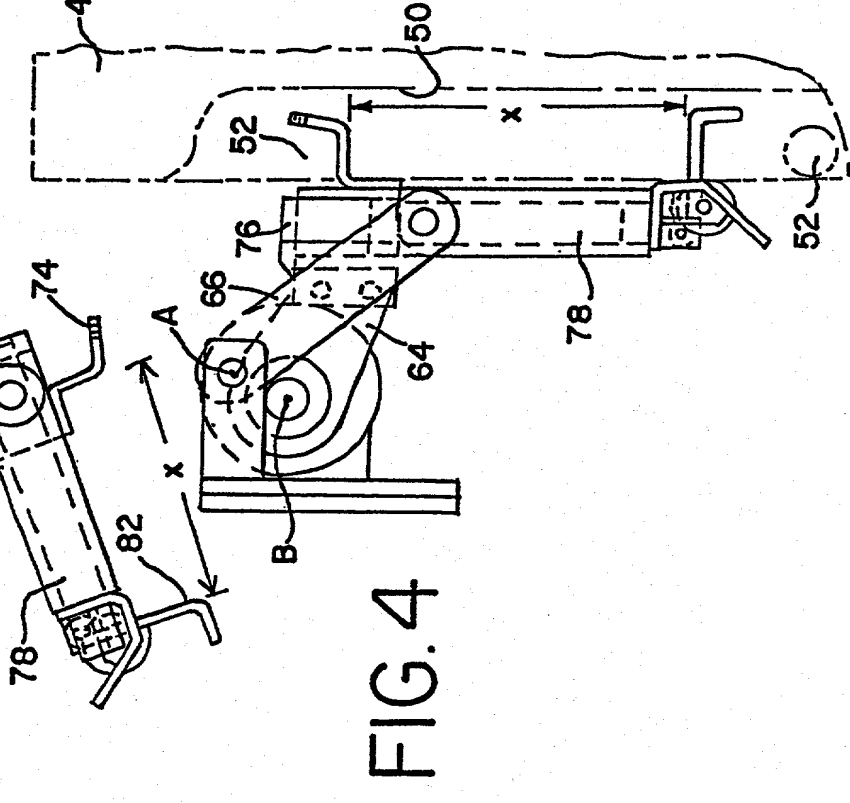



FIG. 4

FIG. 4a




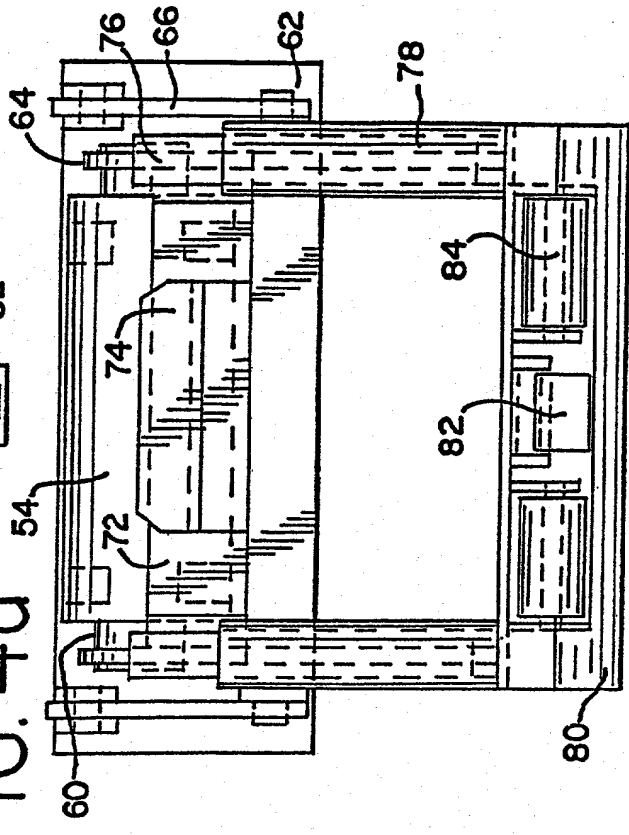


# FIG. 6

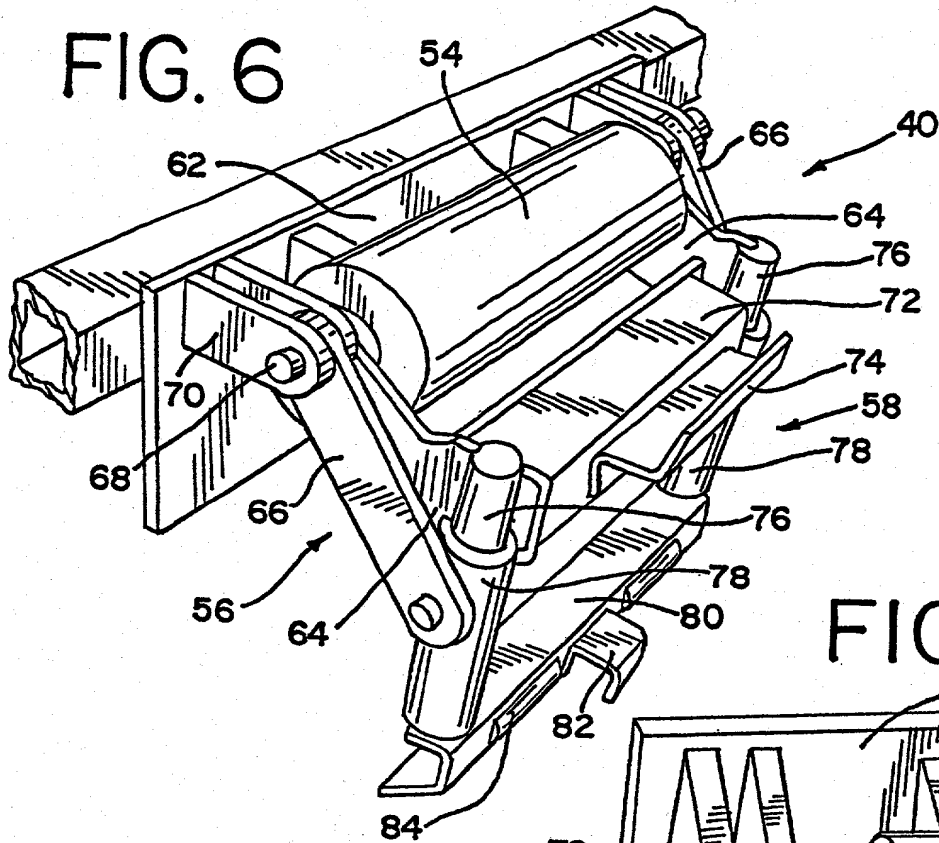


# FIG. 7

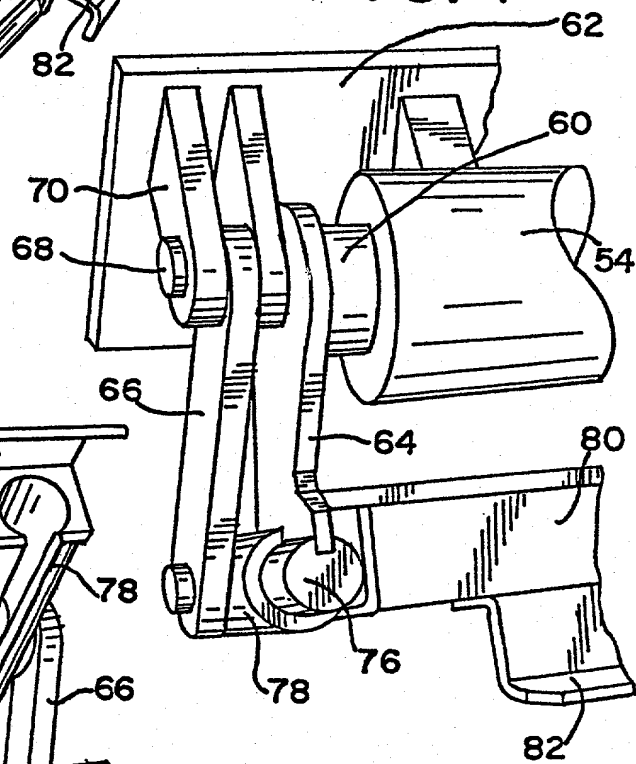


# FIG. 8

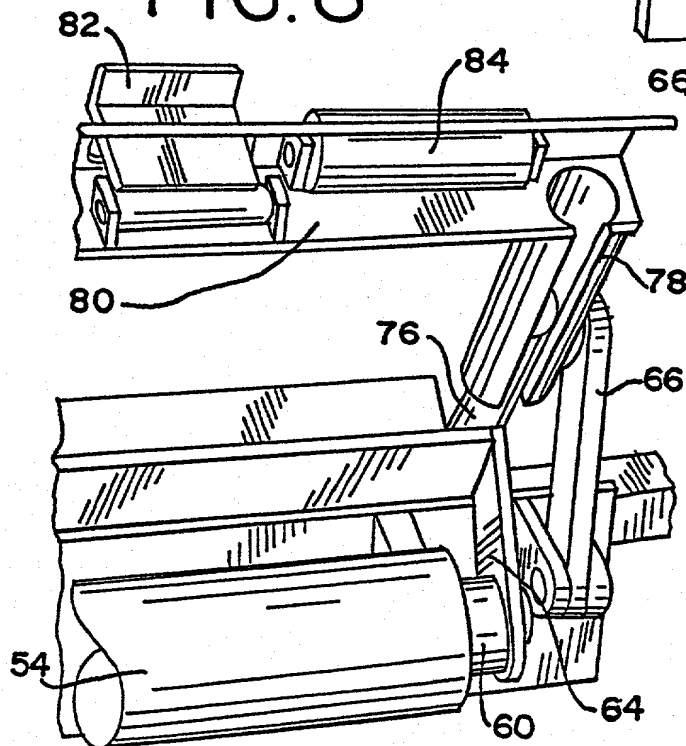

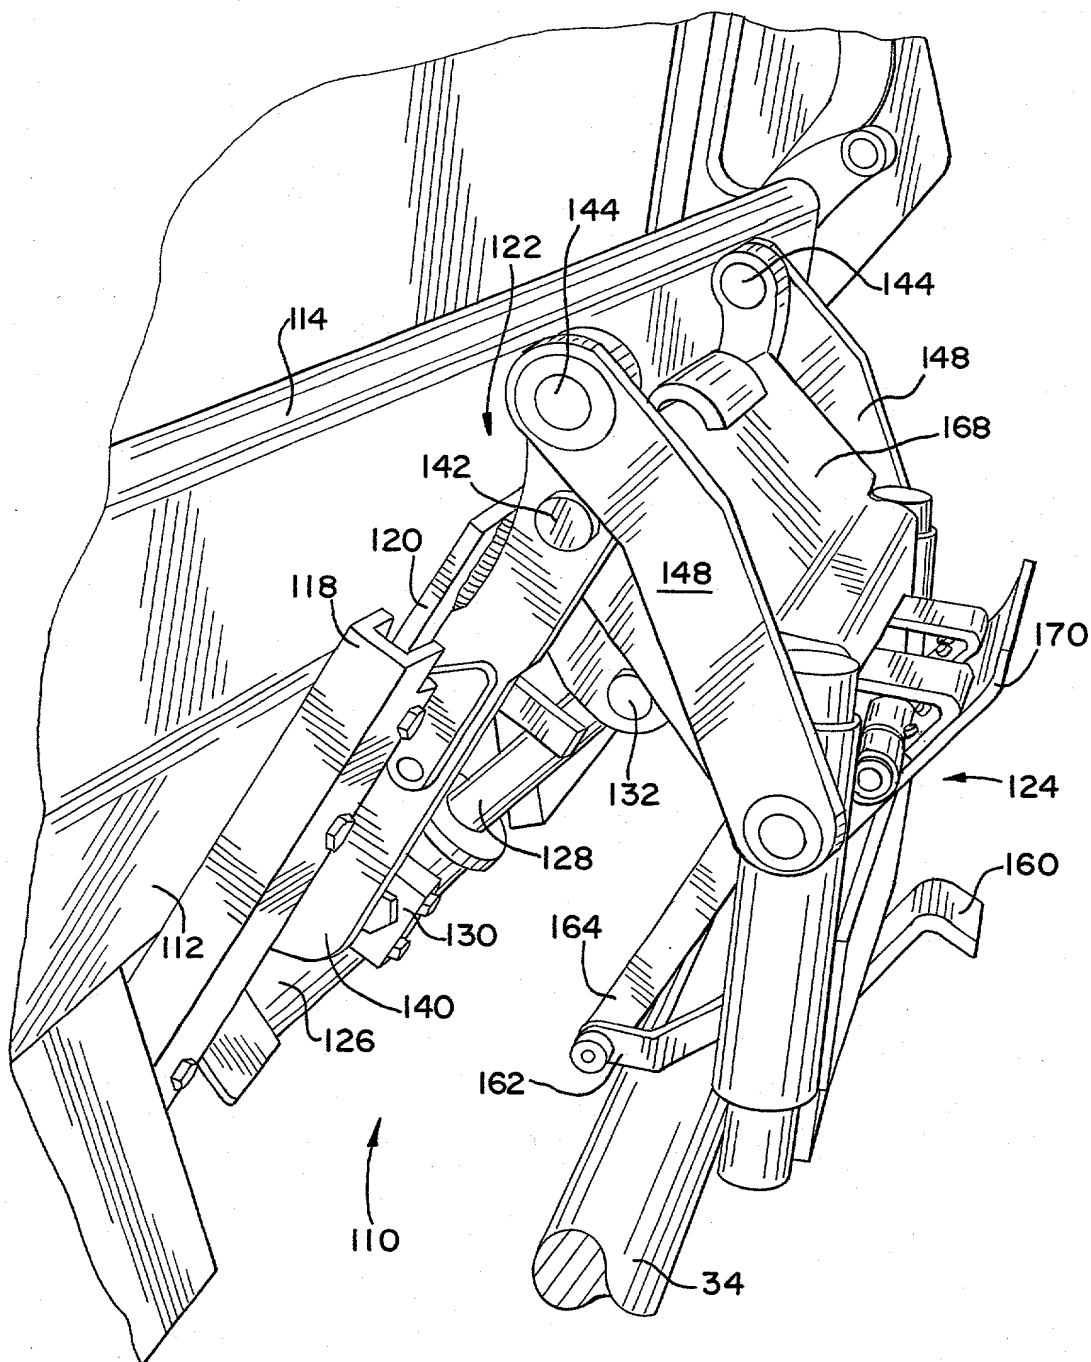

[illegible]

# FIG. 17

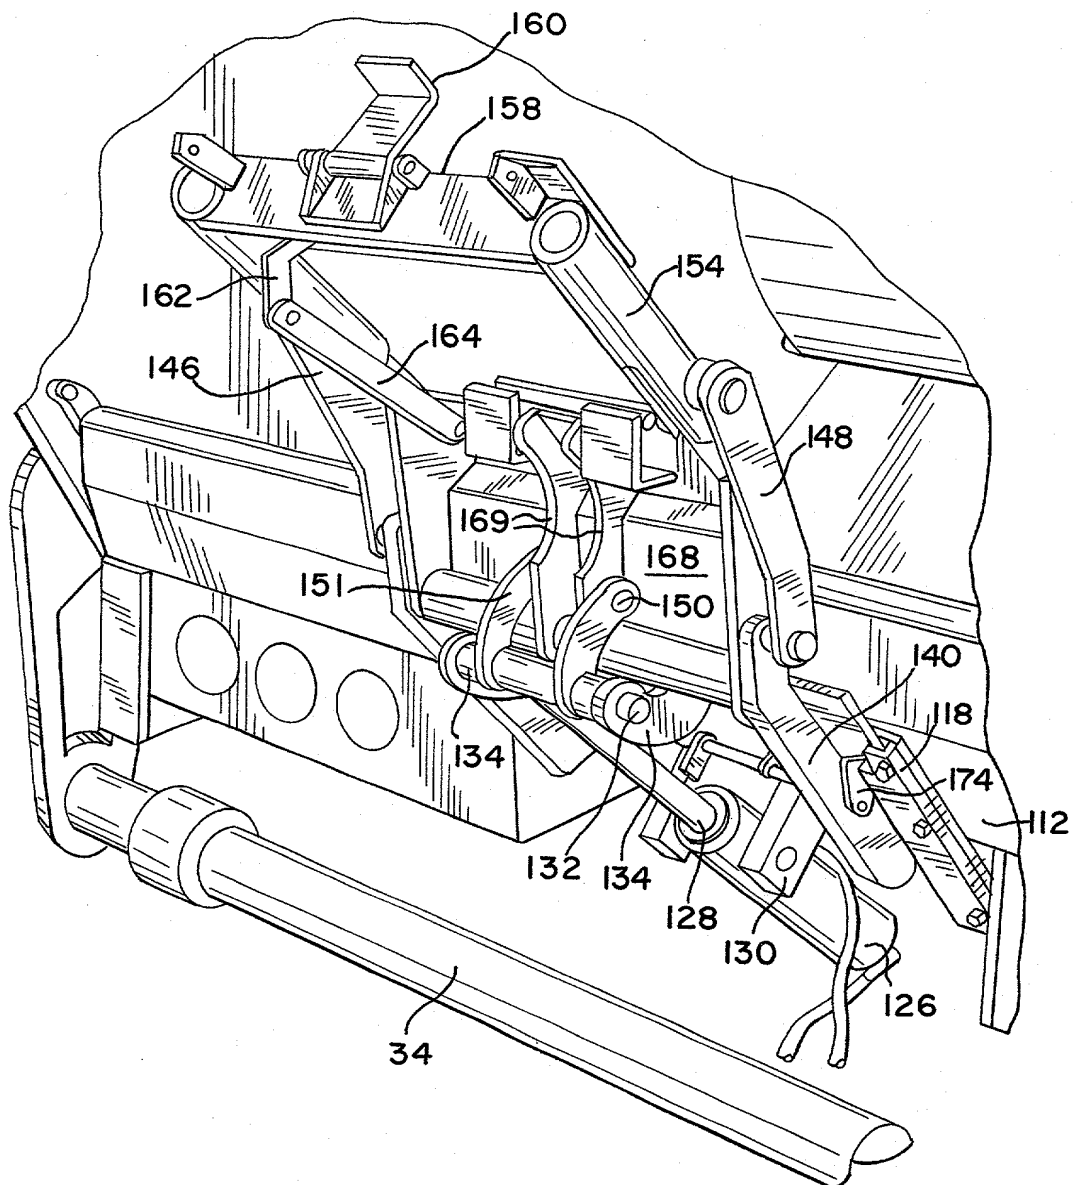

# FIG. 18

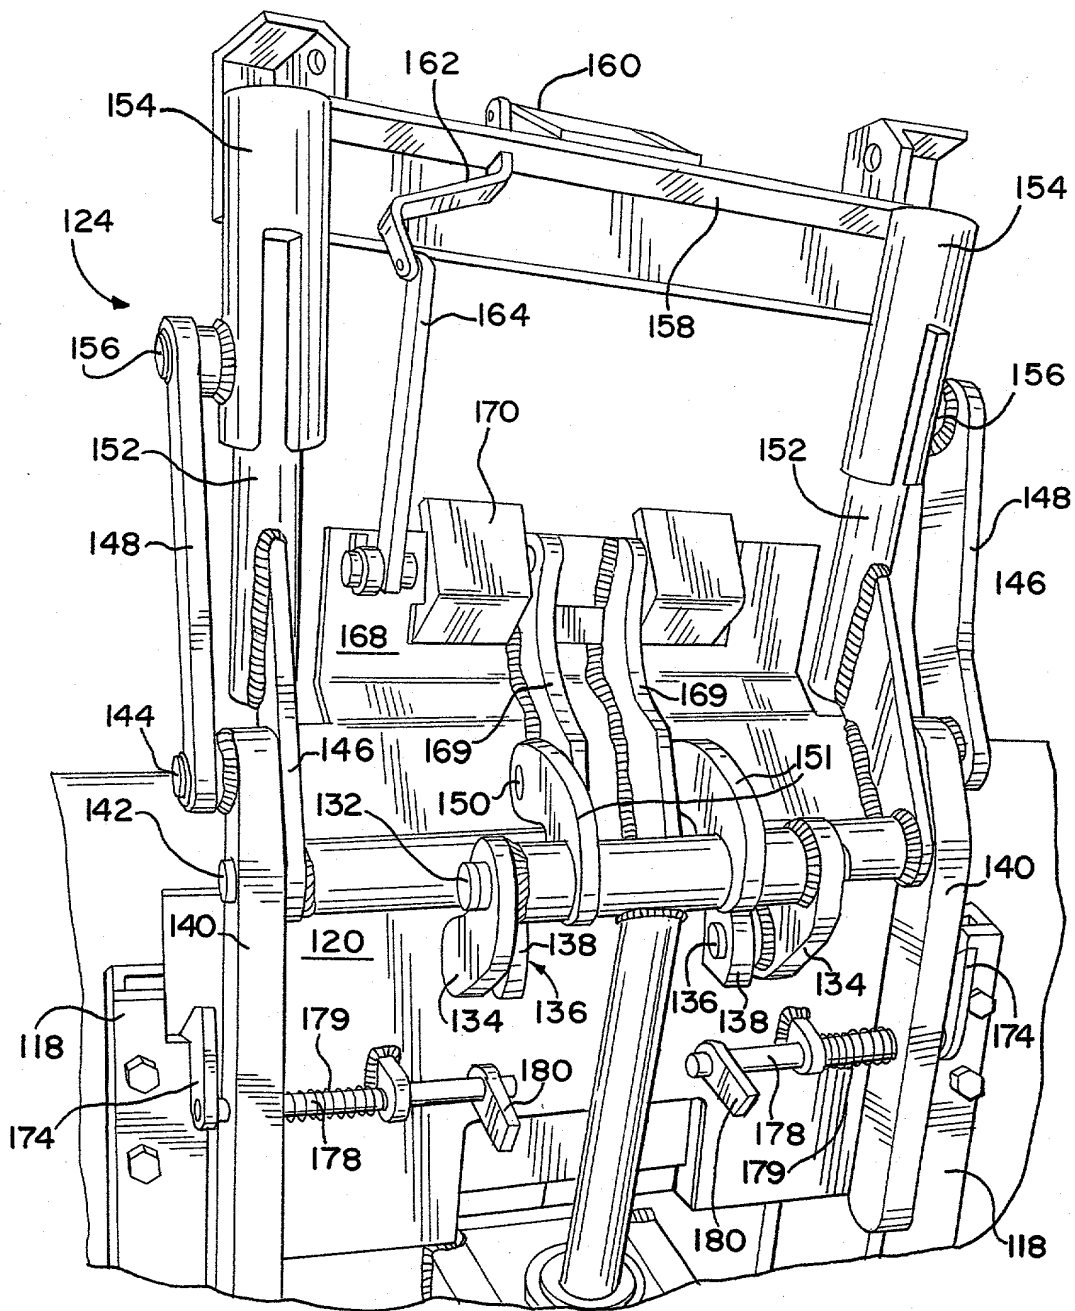




FIG. 19



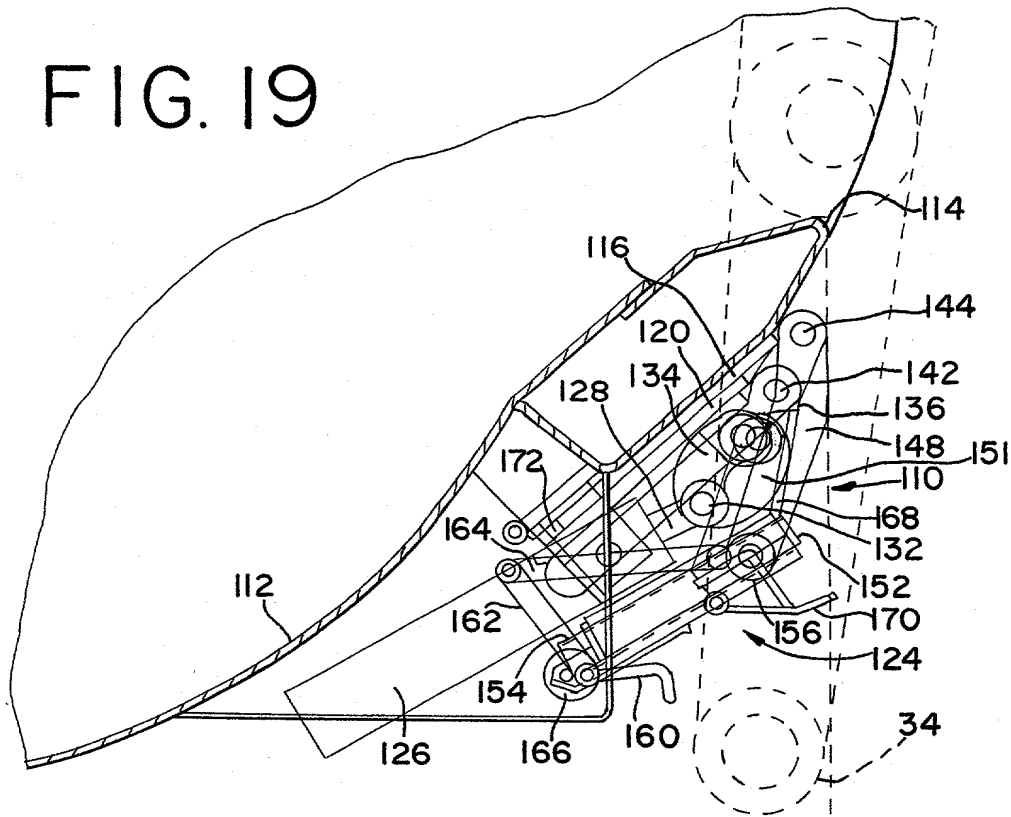


FIG. 20

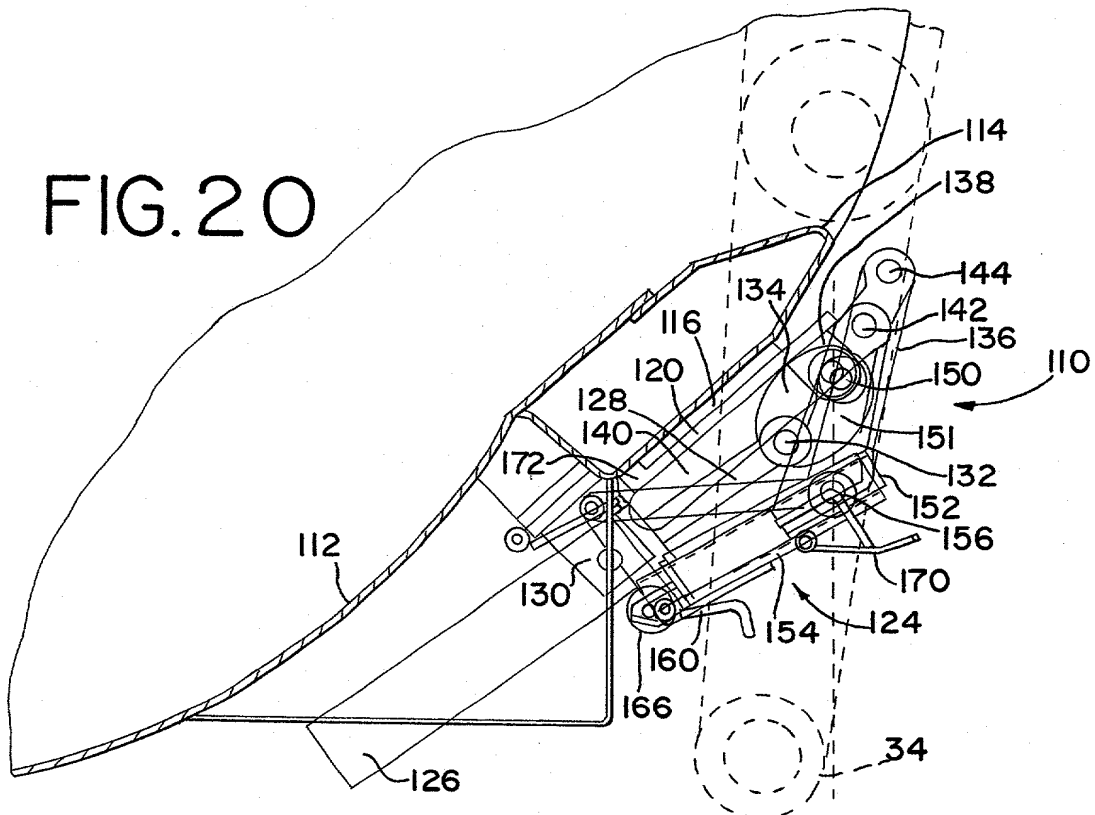

# FIG. 21

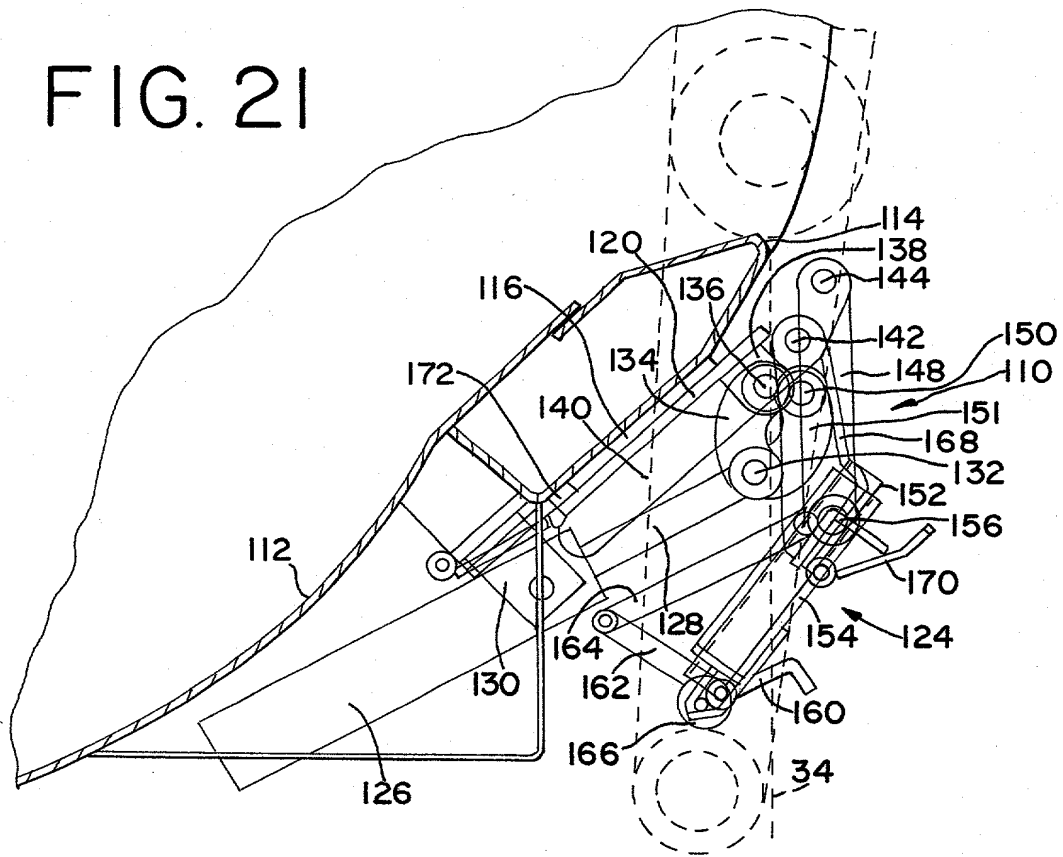

# FIG. 22


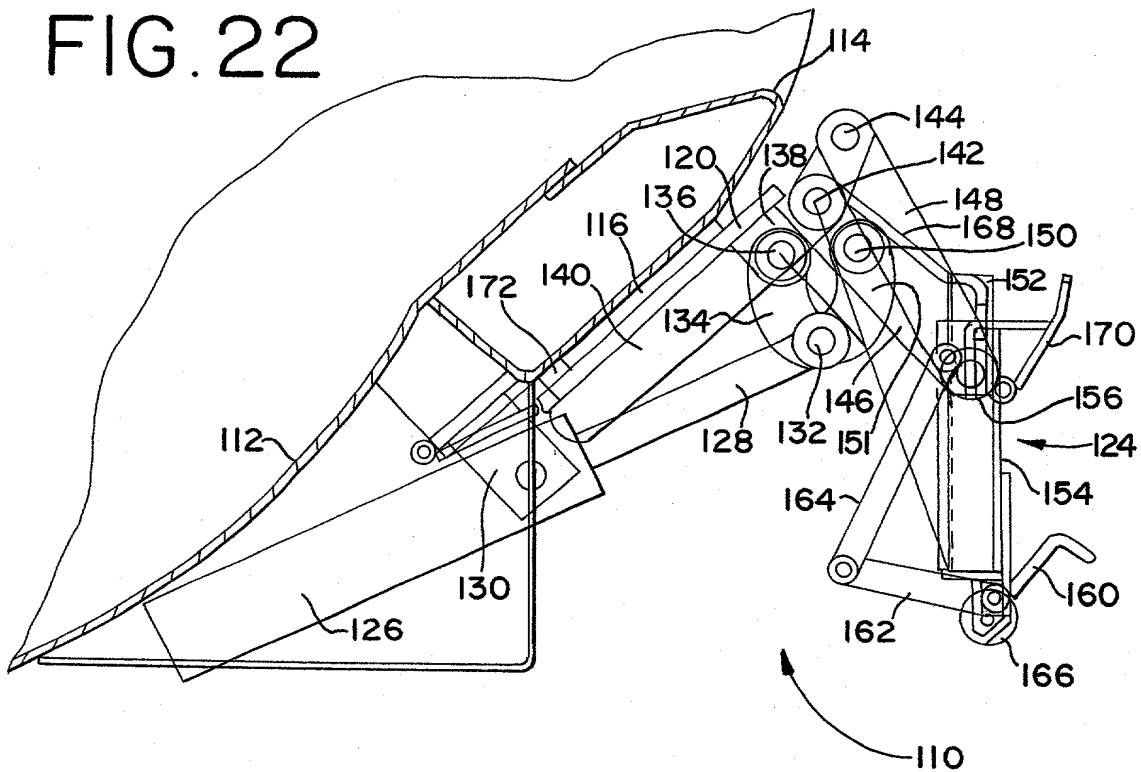


FIG. 23

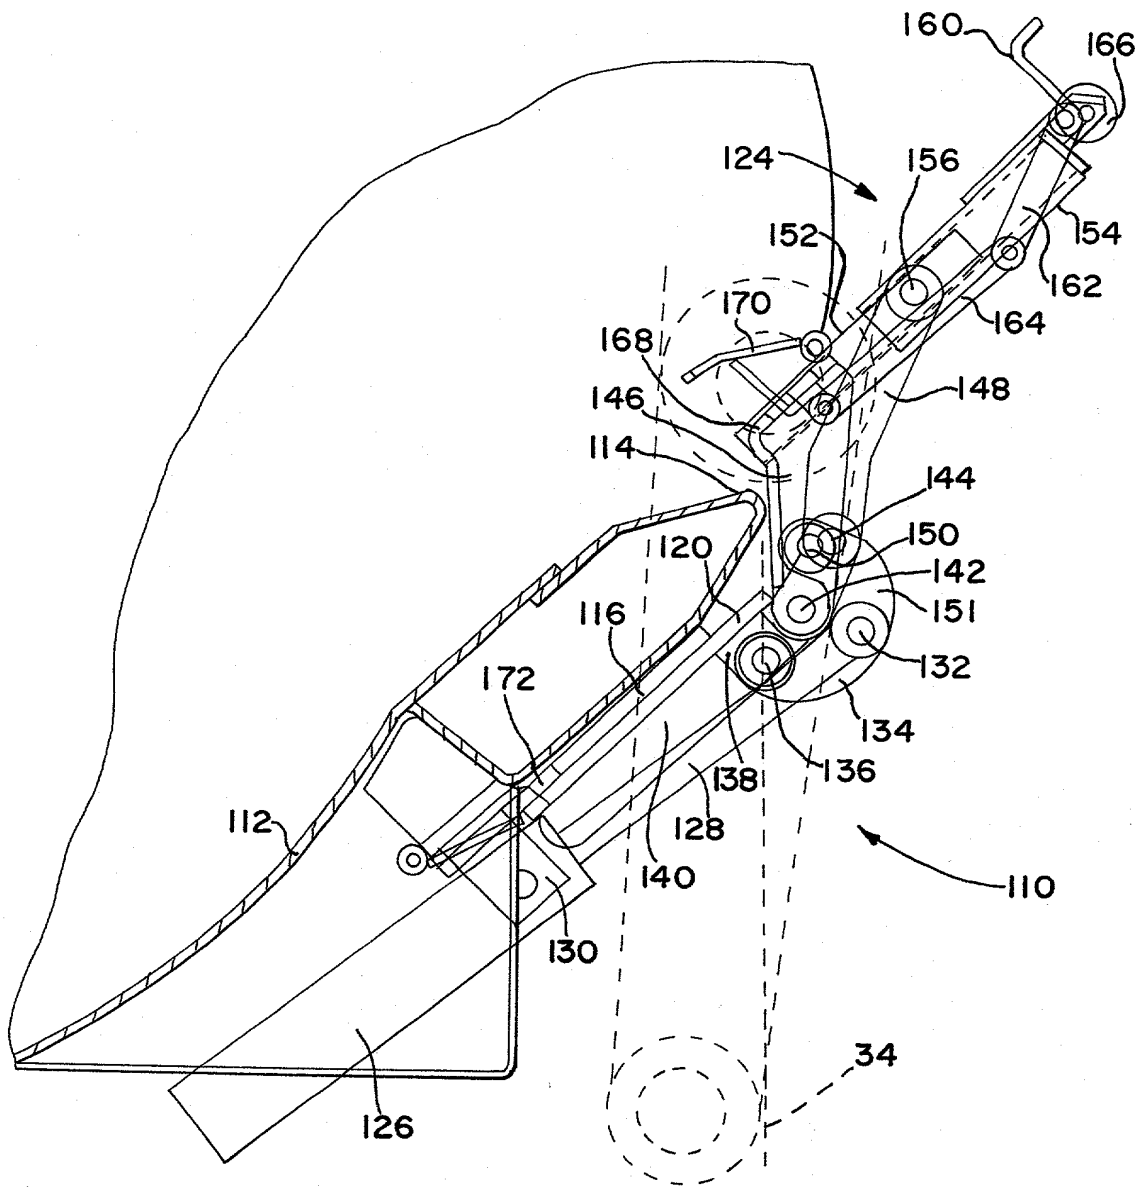

# FIG. 24

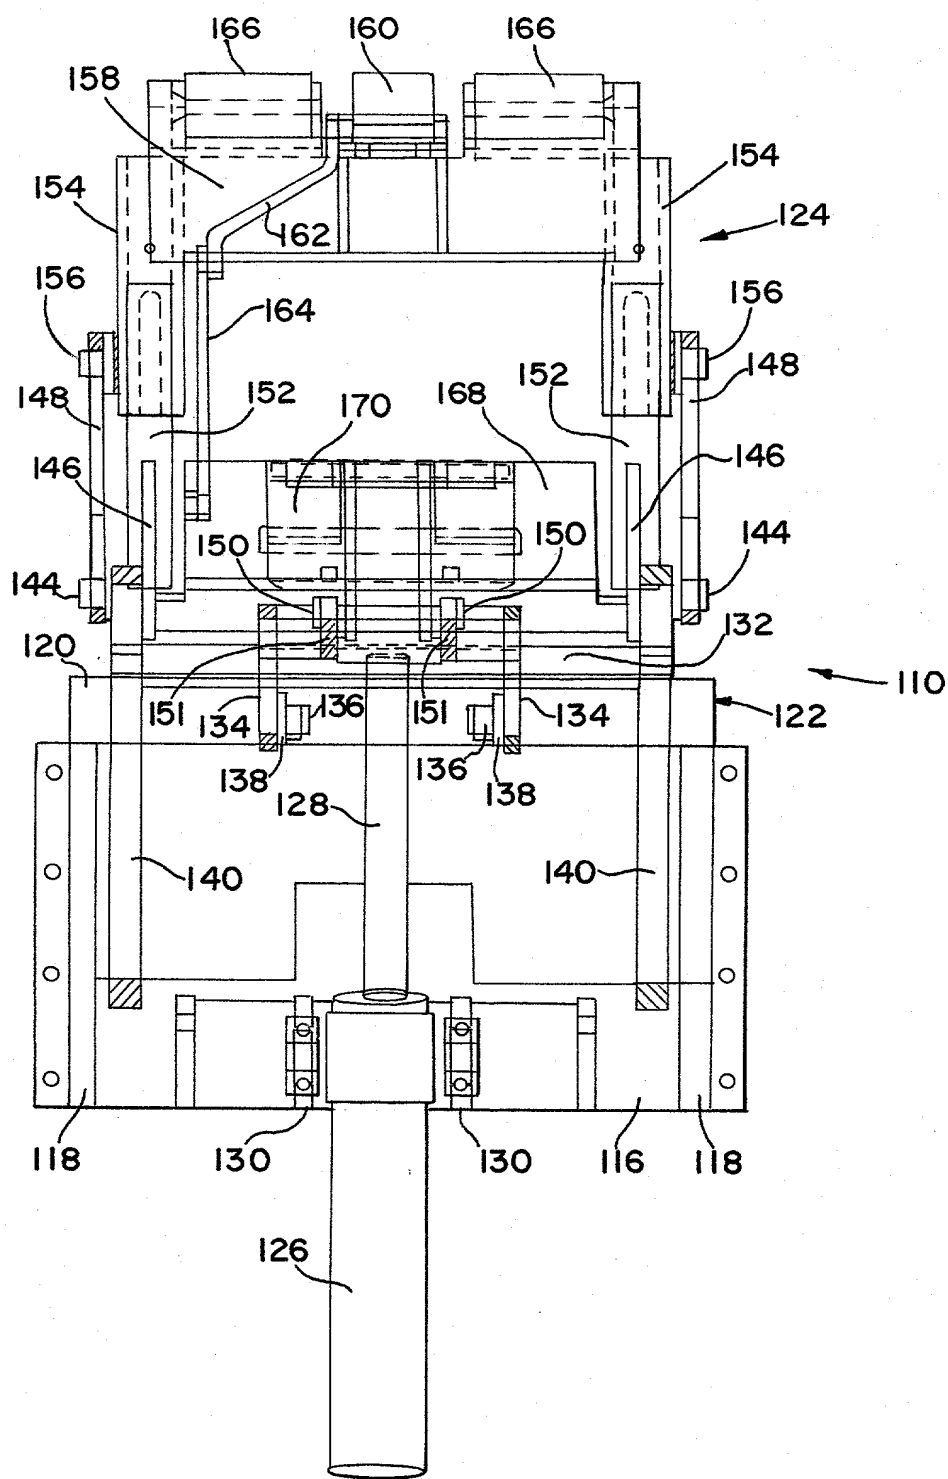


FIG. 25

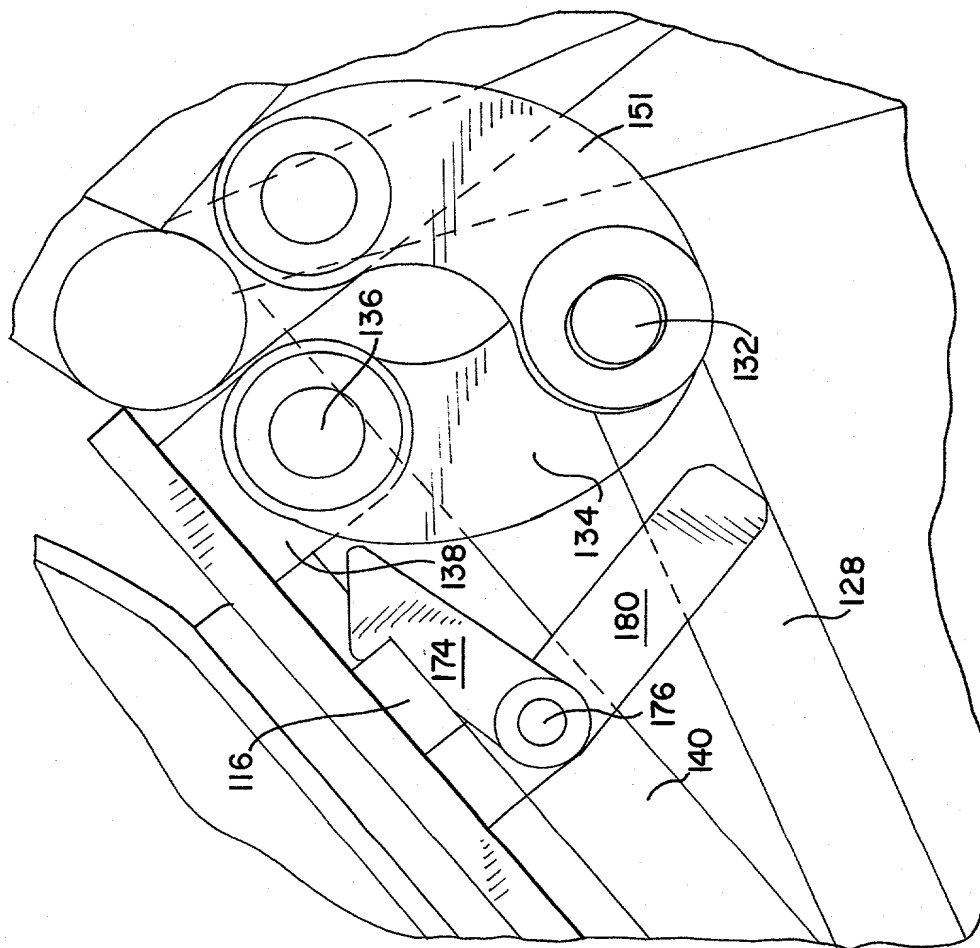


FIG. 26

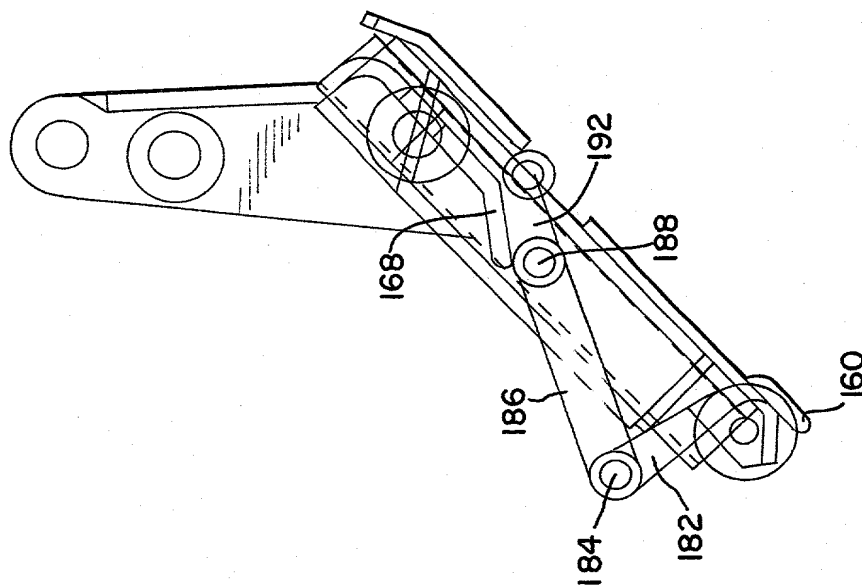


FIG. 27

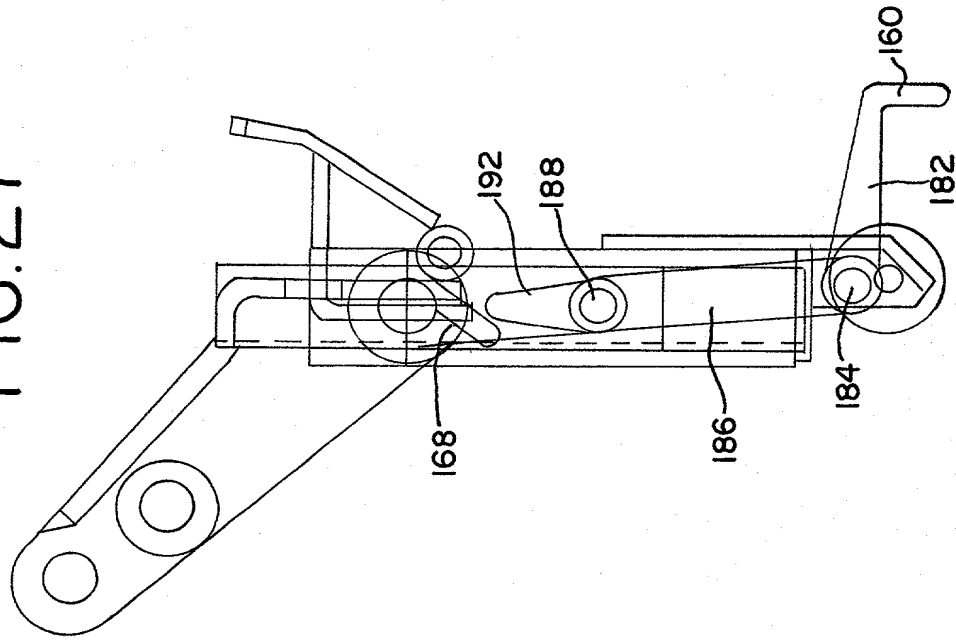


FIG. 28

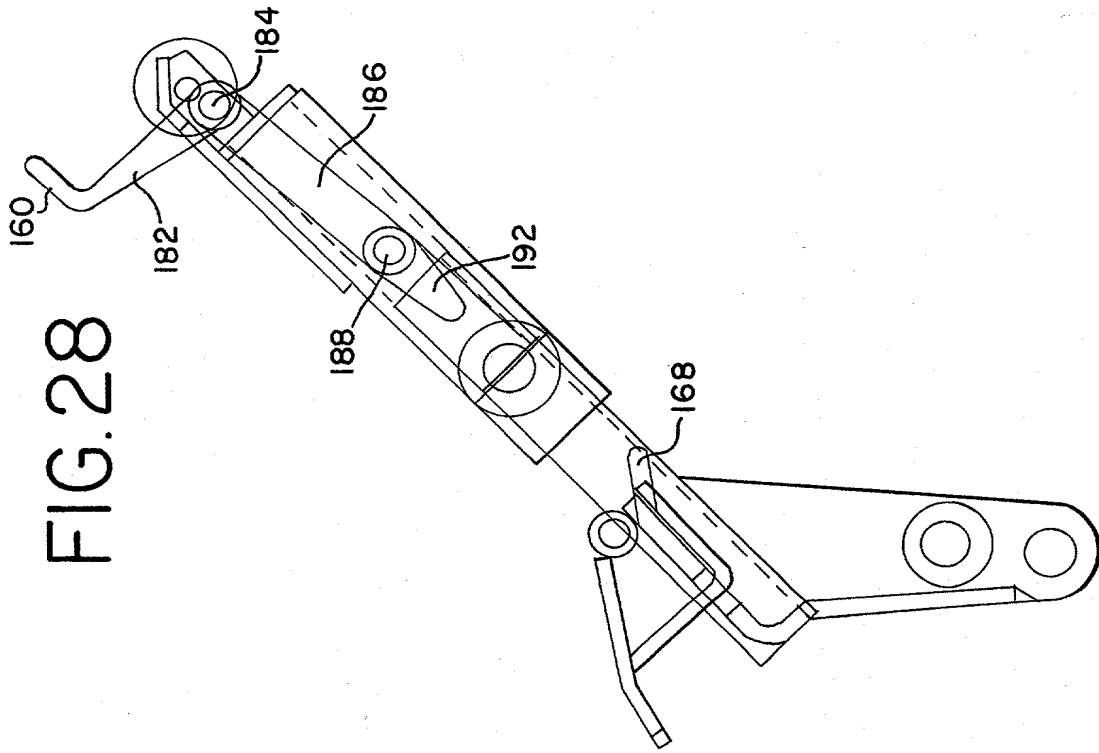


FIG. 29

